


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2127, Rack A, Plate 1, Well F10, 502901
[C823198AC2E3F1BF] Apr 21, 2026 12:08:12 Pressure = 62 bar (62 to 63)

FA

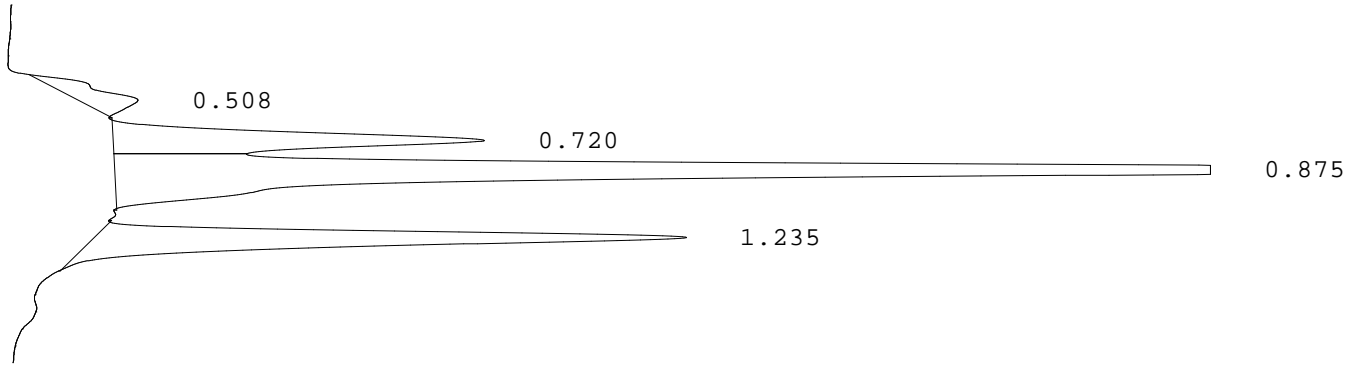

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.508	F 0.59	3.6%	43758	
2	0.720	F 0.83	15.2%	182320	Acetylated F peak
3	0.875	F 1.01	58.8%	705305	Consistent with F
4	1.235	A 1.00	22.4%	268623	A peak - REVIEW

Total Area: 1200006

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range