


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2025, Rack A, Plate 1, Well A10, 490074
[D927956DEE5D7137] Dec 23, 2025 11:21:10 Pressure = 77 bar (77 to 79)

FA

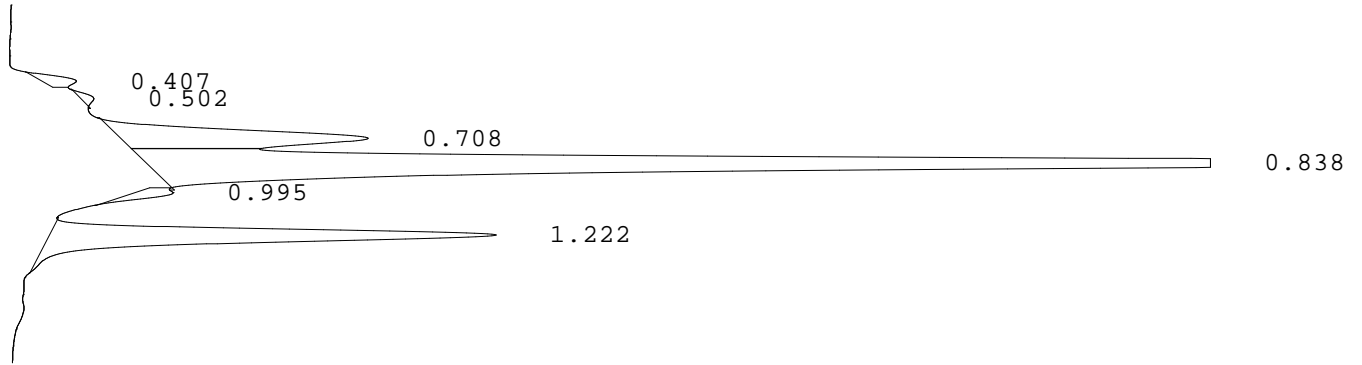

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	1.1%	10234	
2	0.502	F 0.59	0.5%	4508	
3	0.708	F 0.83	12.7%	120067	
4	0.838	F 0.99	65.0%	612397	Acetylated F peak Consistent with F
5	0.995	F 1.17	1.4%	13604	
6	1.222	A 1.01	19.3%	181480	A peak
Total Area:				942290	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range