


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2008, Rack A, Plate 1, Well D09, 171403
[CD73FB3179C5799F] Dec 09, 2025 12:24:40 Pressure = 72 bar (72 to 74)

FA

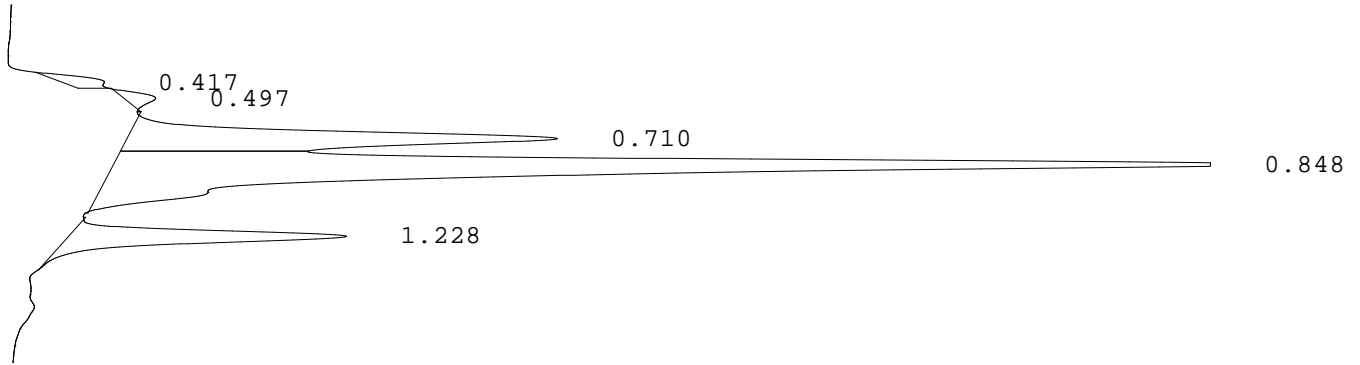

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.417	F 0.48	1.6%	14646	
2	0.497	F 0.57	1.3%	12324	
3	0.710	F 0.82	22.0%	203374	
4	0.848	F 0.98	63.3%	586002	Consistent with F
5	1.228	A 1.01	11.9%	109919	A peak
Total Area:				926265	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range