


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2182, Rack A, Plate 1, Well A05, 503326
[D93DAF2DC61064CA] Jun 23, 2026 10:17:12 Pressure = 72 bar (72 to 75)

FA

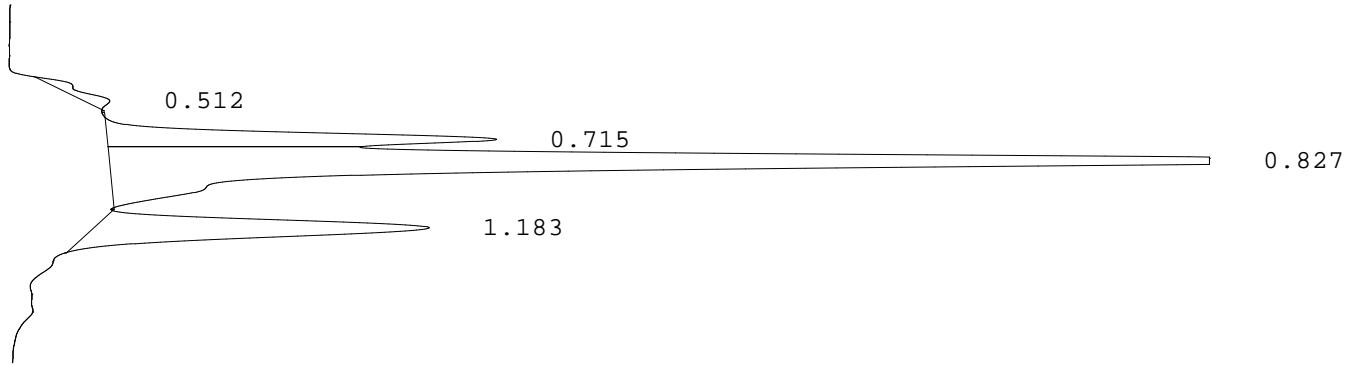

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.512	F 0.61	1.7%	17111	
2	0.715	F 0.86	14.8%	151154	Acetylated F peak
3	0.827	F 0.99	66.0%	674516	Consistent with F
4	1.183	A 1.01	17.5%	179299	A peak
Total Area:				1022080	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range