


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2022, Rack A, Plate 1, Well B10, 171540
 [8C77D5867500AE62] Dec 19, 2025 10:48:22 Pressure = 75 bar (75 to 77)

FA

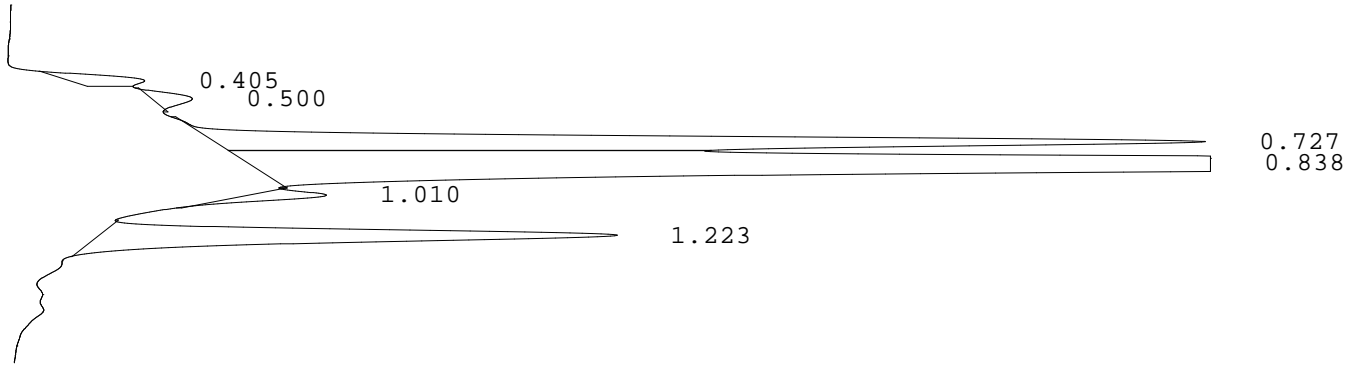

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.48	1.4%	22863	
2	0.500	F 0.59	0.9%	15791	
3	0.727	F 0.86	20.9%	348889	
4	0.838	F 0.99	63.2%	1053481	Consistent with F
5	1.010	F 1.19	1.5%	24336	
6	1.223	A 1.01	12.0%	200505	A peak
Total Area:				1665865	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range