


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2143, Rack A, Plate 1, Well D01, 496518  
[DC775B4949E1D9B7] May 08, 2026 12:38:38 Pressure = 63 bar (63 to 65)

FA

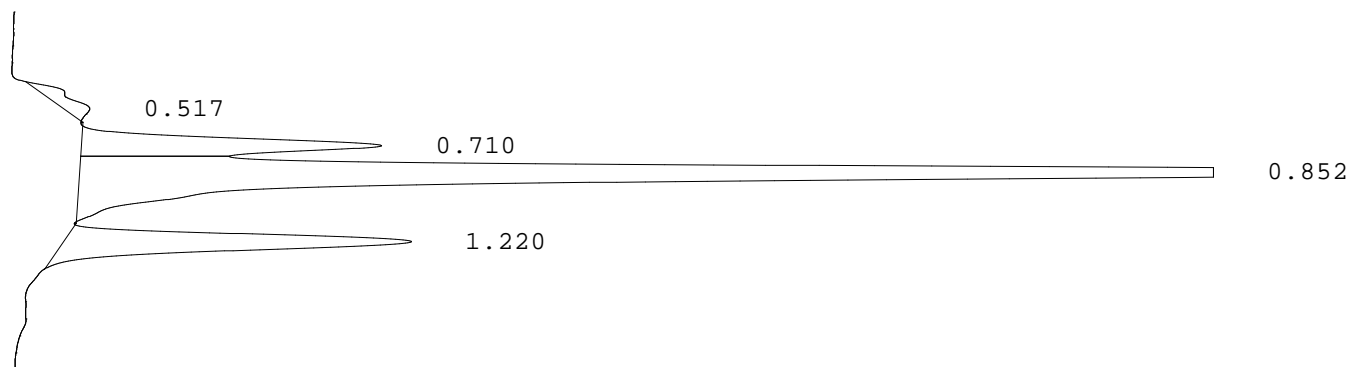

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.517	F 0.60	2.0%	21572	
2	0.710	F 0.83	12.6%	135491	Acetylated F peak
3	0.852	F 0.99	69.4%	746320	Consistent with F
4	1.220	A 1.02	16.0%	172357	A peak
Total Area:				1075740	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range