


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 1993, Rack A, Plate 1, Well C12, 483303  
[CD73A992FDB82E68] Nov 25, 2025 11:45:57 Pressure = 69 bar (68 to 70)

FA

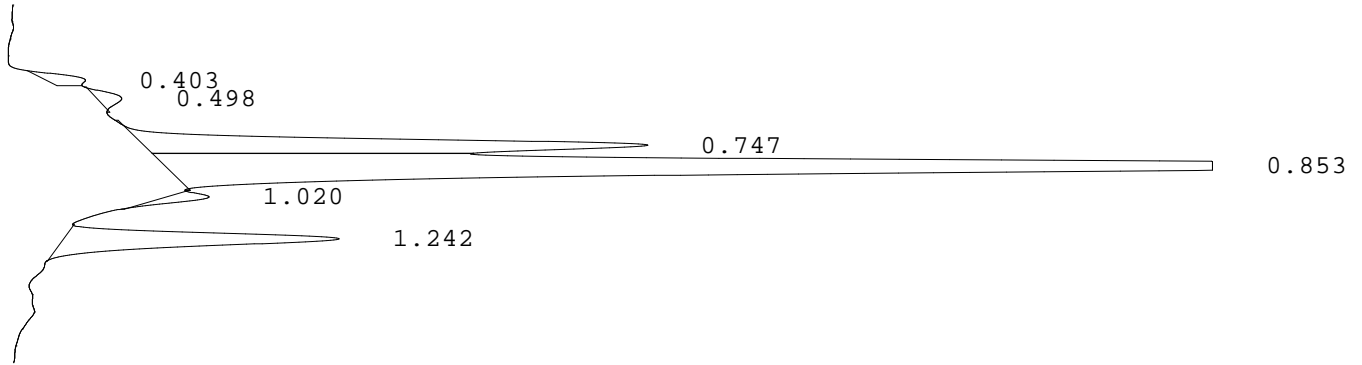

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.46	1.3%	12156	
2	0.498	F 0.57	1.1%	10456	
3	0.747	F 0.85	20.3%	193033	
4	0.853	F 0.97	64.3%	613004	Consistent with F
5	1.020	F 1.16	1.4%	13779	
6	1.242	A 1.01	11.6%	110730	A peak
Total Area:				953158	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range