


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2080, Rack A, Plate 1, Well C10, 492108
[8C273312FC068648] Feb 24, 2026 11:32:33 Pressure = 56 bar (56 to 58)

FA

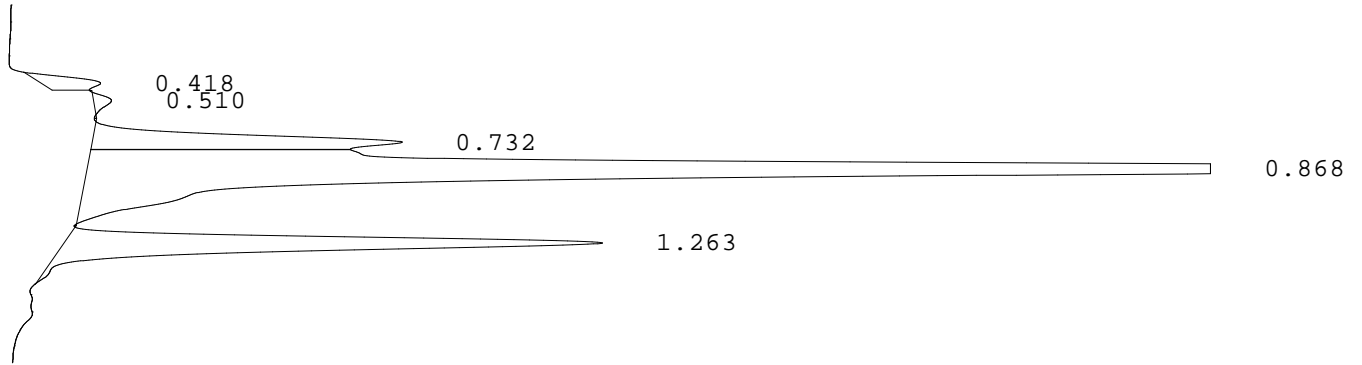

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.418	F 0.48	1.7%	20556	
2	0.510	F 0.58	0.6%	7567	
3	0.732	F 0.83	10.6%	128199	Acetylated F peak
4	0.868	F 0.99	68.4%	829415	Consistent with F
5	1.263	A 1.01	18.7%	227170	A peak
Total Area:				1212907	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range