


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 1380, Rack A, Plate 1, Well D10, 27420  
 [9D99A24EE1F0CA4A] Apr 17, 2024 11:57:36 Pressure = 88 bar (88 to 89)

FA

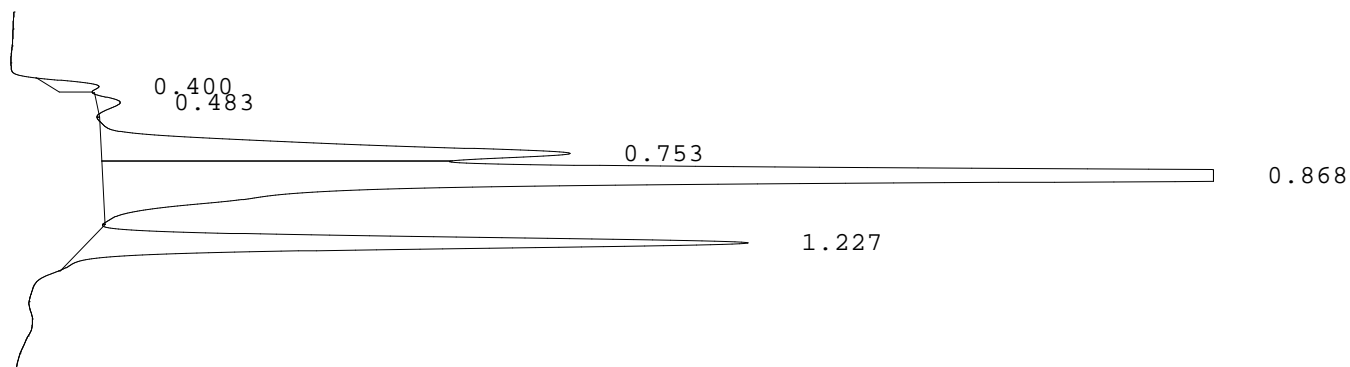

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.400	F 0.46	1.0%	14249	
2	0.483	F 0.56	0.6%	8684	
3	0.753	F 0.87	16.4%	228546	Acetylated F peak
4	0.868	F 1.00	64.0%	889178	Consistent with F
5	1.227	A 1.01	18.0%	249572	A peak
Total Area:				1390229	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range