


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2029, Rack A, Plate 1, Well H01, 490092  
[8D6386B8BAAA26CA] Dec 29, 2025 13:46:00 Pressure = 73 bar (73 to 75)

FA

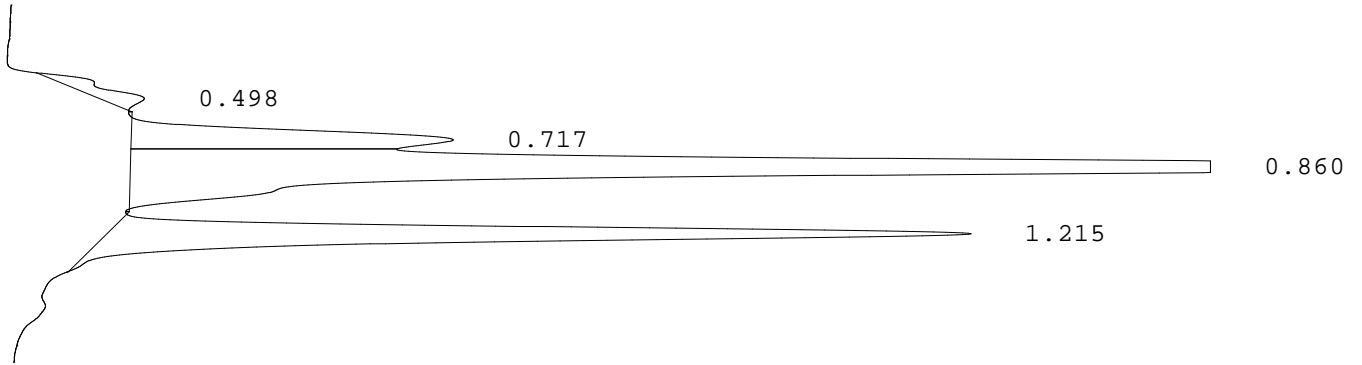

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.498	F 0.58	2.2%	32026	
2	0.717	F 0.83	11.7%	170378	Acetylated F peak
3	0.860	F 1.00	59.1%	860060	Consistent with F
4	1.215	A 1.00	27.0%	392394	A peak - REVIEW
Total Area:				1454858	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range