


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1380, Rack A, Plate 1, Well D09, 27419
[88CDA24EE1F04A60] Apr 17, 2024 11:55:35

Pressure = 88 bar (88 to 88)

FA

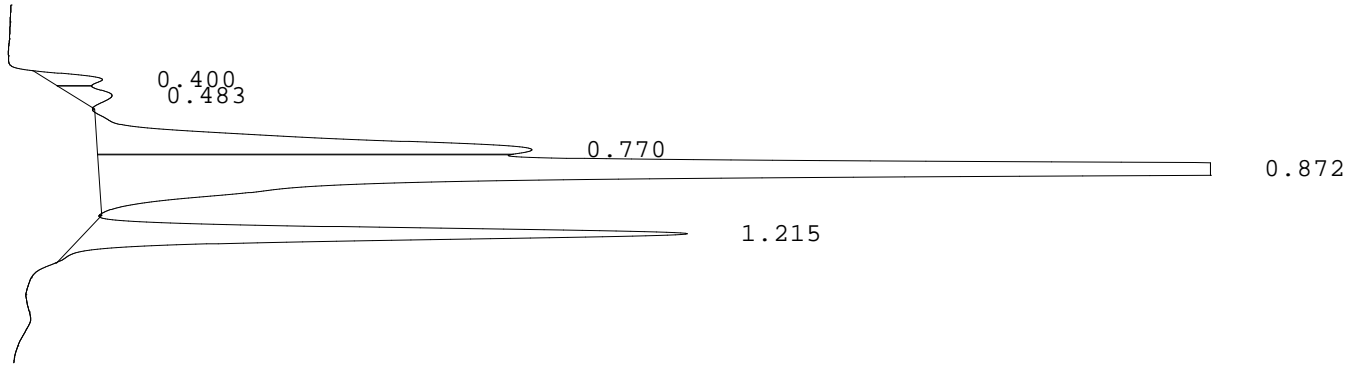

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.400	F 0.46	1.1%	17068	
2	0.483	F 0.56	1.2%	18416	
3	0.770	F 0.89	14.6%	222170	Acetylated F peak
4	0.872	F 1.00	67.6%	1027976	Consistent with F
5	1.215	A 1.00	15.4%	234894	A peak
Total Area:				1520524	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range