


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2025, Rack A, Plate 1, Well A09, 490073
[D873C038BB0AA4E8] Dec 23, 2025 11:19:09 Pressure = 77 bar (77 to 79)

FA

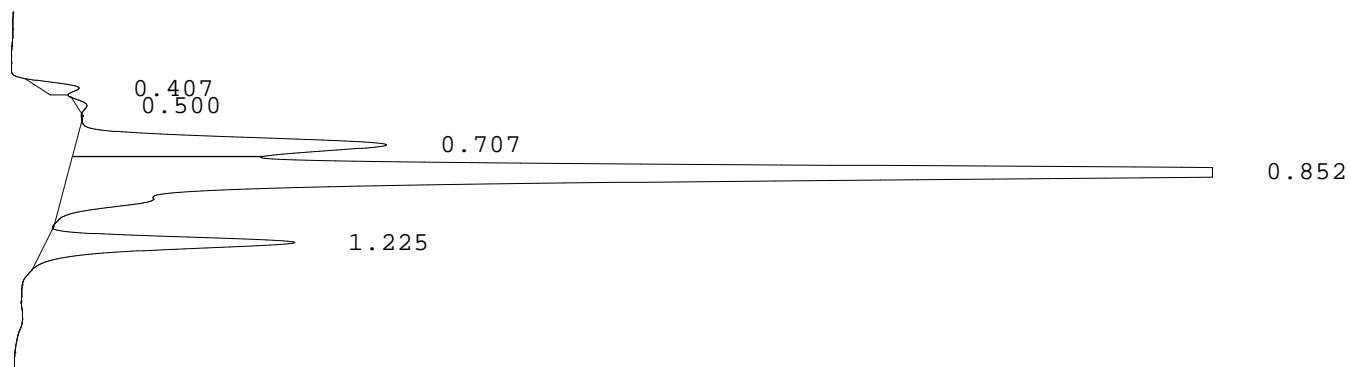

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	1.2%	12071	
2	0.500	F 0.59	0.4%	3622	
3	0.707	F 0.83	15.4%	157339	Acetylated F peak
4	0.852	F 1.00	73.4%	749300	Consistent with F
5	1.225	A 1.01	9.6%	98183	A peak

Total Area: 1020515

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range