


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2179, Rack A, Plate 1, Well D12, 503047
[8C39EF942A12EE42] Jun 18, 2026 14:10:58 Pressure = 71 bar (70 to 72)

FA

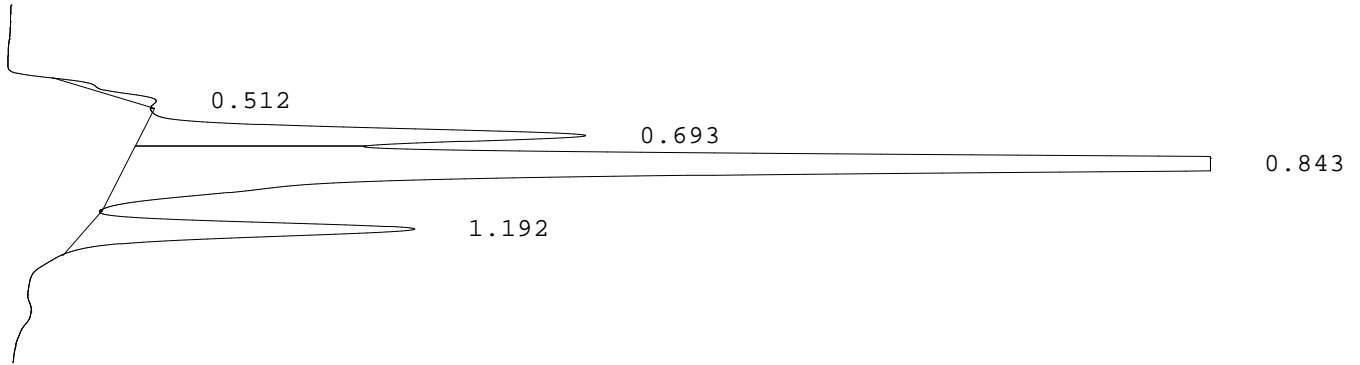

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.512	F 0.61	1.2%	16308	
2	0.693	F 0.83	15.1%	208074	Acetylated F peak
3	0.843	F 1.01	72.7%	1001157	Consistent with F
4	1.192	A 1.00	11.0%	151238	A peak
Total Area:				1376777	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range