


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1977, Rack A, Plate 1, Well B11, 171013
[9C63A78E680FD317] Nov 14, 2025 10:54:10 Pressure = 69 bar (68 to 70)

FA

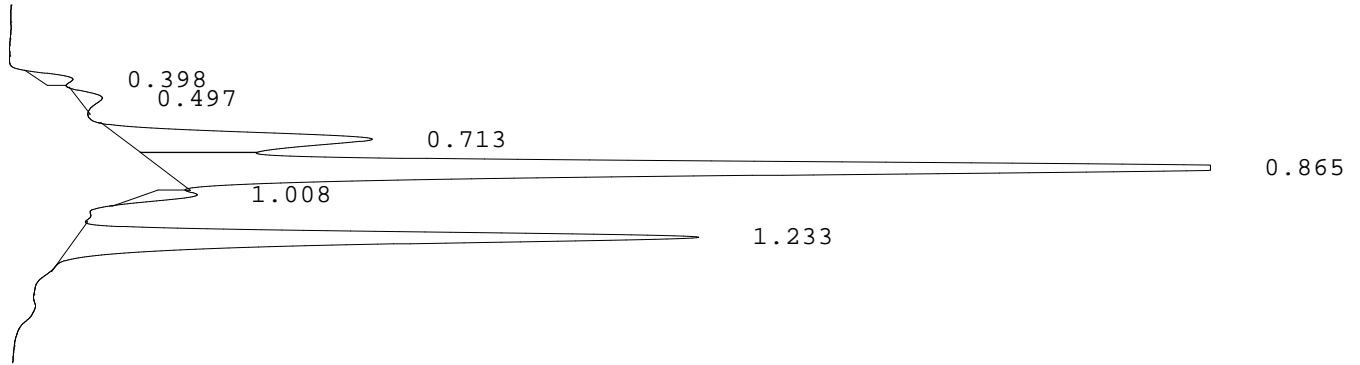

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.398	F 0.46	1.2%	10530	
2	0.497	F 0.58	1.1%	10211	
3	0.713	F 0.83	13.6%	122333	Acetylated F peak
4	0.865	F 1.01	55.4%	499429	Consistent with F
5	1.008	F 1.17	1.9%	16740	
6	1.233	A 1.01	26.9%	242277	A peak - REVIEW
Total Area:				901520	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range