


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2025, Rack A, Plate 1, Well E02, 490112
[8D36906DEC7FF317] Dec 23, 2025 12:44:02 Pressure = 75 bar (75 to 77)

FA

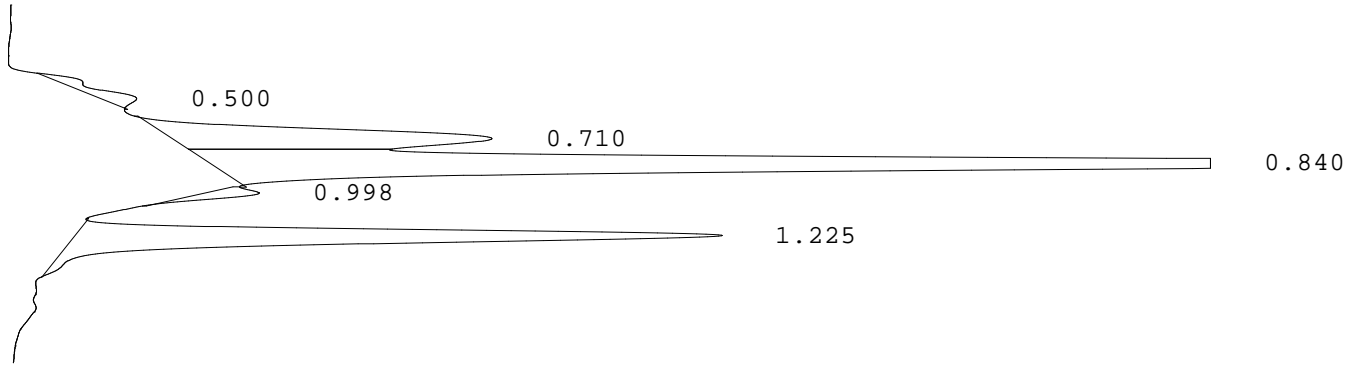

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.500	F 0.59	2.1%	23021	
2	0.710	F 0.83	15.9%	176125	Acetylated F peak
3	0.840	F 0.99	55.5%	615611	Consistent with F
4	0.998	F 1.17	1.7%	18731	
5	1.225	A 1.00	24.8%	275148	A peak - REVIEW

Total Area: 1108636

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range