


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1889, Rack A, Plate 1, Well D10, 830805
[D97539DC1F3B26E0] Aug 20, 2025 12:22:55 Pressure = 59 bar (59 to 60)

FA

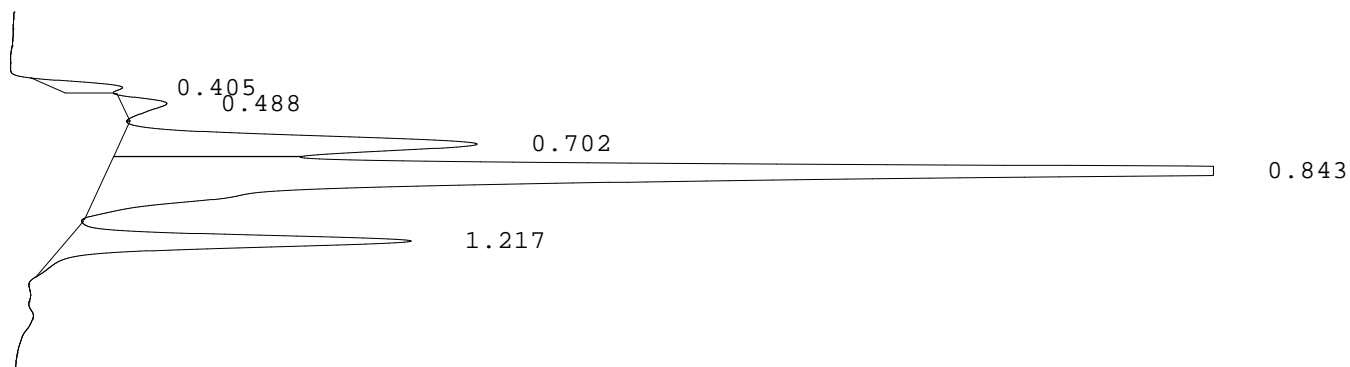

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.48	1.8%	20767	
2	0.488	F 0.58	1.6%	18475	
3	0.702	F 0.83	16.8%	190096	Acetylated F peak
4	0.843	F 0.99	67.4%	764518	Consistent with F
5	1.217	A 1.01	12.3%	139876	A peak
Total Area:				1133732	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range