


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1993, Rack A, Plate 1, Well A04, 482028
[8D72FC92FFB88640] Nov 25, 2025 10:39:15 Pressure = 70 bar (70 to 72)

FA

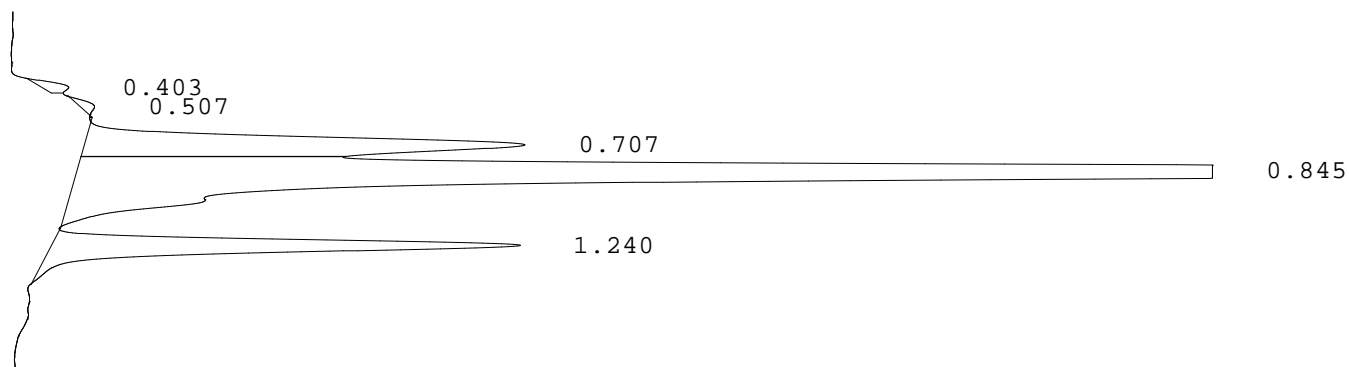

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.47	0.5%	7900	
2	0.507	F 0.59	0.4%	5685	
3	0.707	F 0.82	14.8%	225116	Acetylated F peak
4	0.845	F 0.99	71.9%	1091149	Consistent with F
5	1.240	A 1.02	12.4%	187484	A peak
Total Area:				1517334	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range