


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2034, Rack A, Plate 1, Well B06, 490099
[CD238703017F5915] Jan 06, 2026 11:10:59 Pressure = 83 bar (82 to 85)

FA

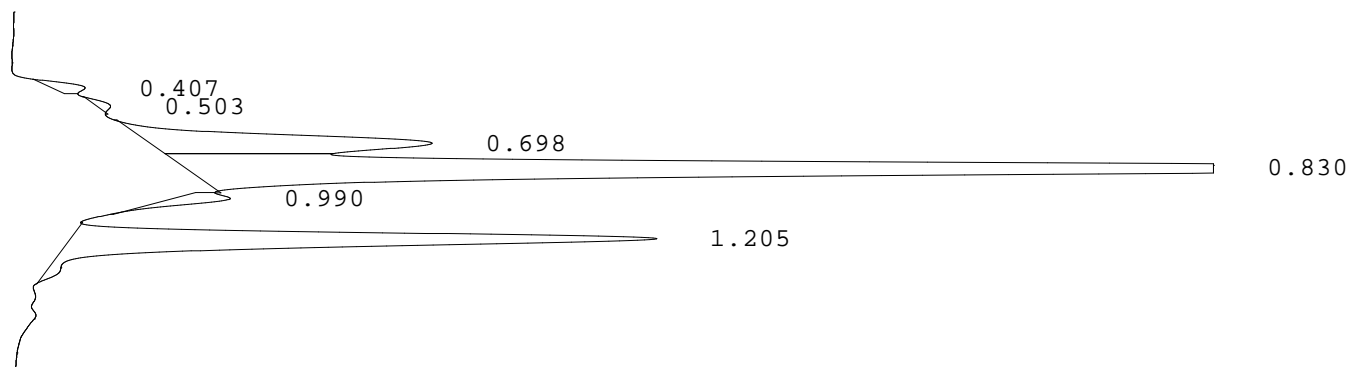

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.49	0.9%	9580	
2	0.503	F 0.60	0.4%	4669	
3	0.698	F 0.83	13.7%	143470	Acetylated F peak
4	0.830	F 0.99	59.0%	619431	Consistent with F
5	0.990	F 1.18	2.0%	20594	
6	1.205	A 1.02	24.0%	252443	A peak - REVIEW

Total Area: 1050187

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range