


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2025, Rack A, Plate 1, Well E11, 490121
 [C8738138B9888CE0] Dec 23, 2025 13:04:15 Pressure = 75 bar (75 to 77)

FA

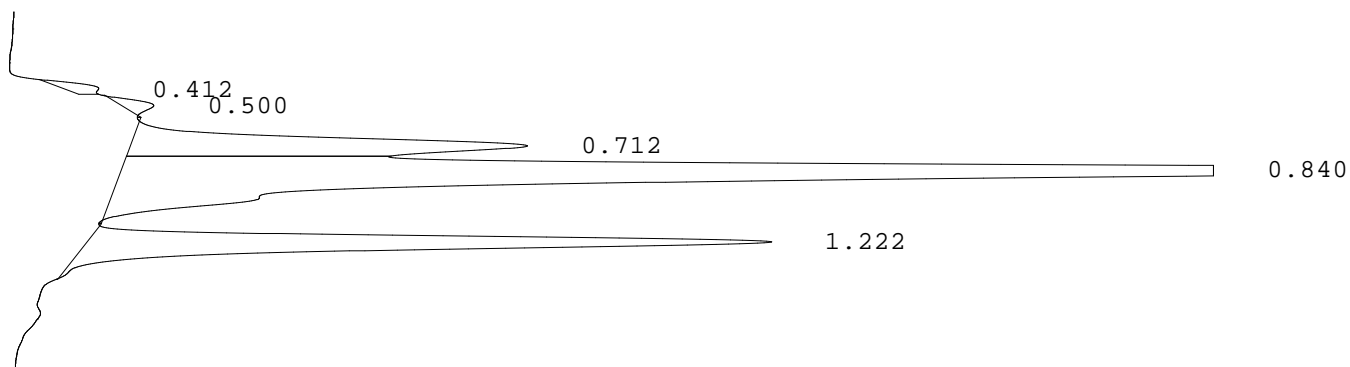

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.412	F 0.47	0.8%	11100	
2	0.500	F 0.58	0.9%	11918	
3	0.712	F 0.82	14.6%	199268	Acetylated F peak
4	0.840	F 0.97	62.4%	849724	Consistent with F
5	1.222	A 1.01	21.3%	290078	A peak - REVIEW
Total Area:				1362088	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range