


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2049, Rack A, Plate 1, Well B07, 488992  
[8D33CD5F96E2AC4A] Jan 20, 2026 11:35:28 Pressure = 81 bar (81 to 83)

FA

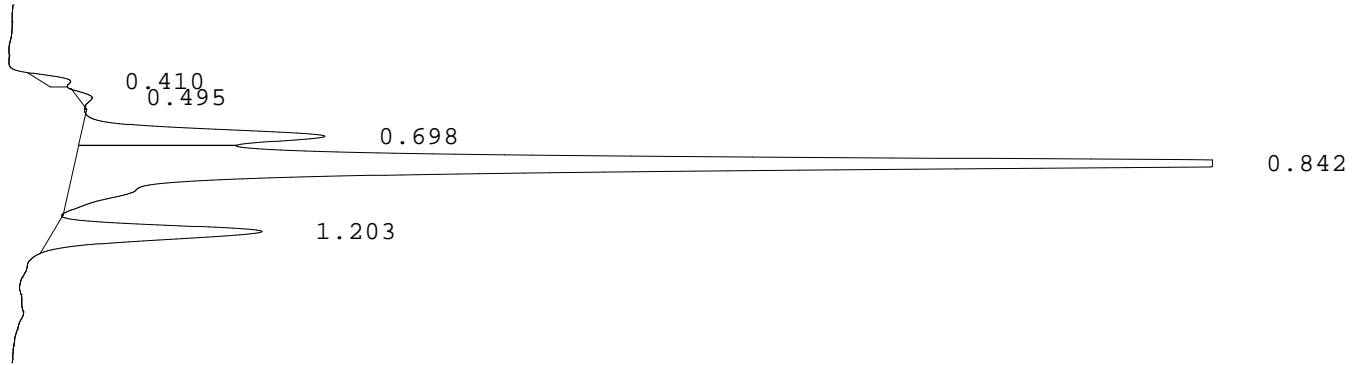

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.410	F 0.49	1.0%	8753	
2	0.495	F 0.59	0.6%	4926	
3	0.698	F 0.83	12.5%	108900	Acetylated F peak
4	0.842	F 1.00	75.1%	652859	Consistent with F
5	1.203	A 1.02	10.8%	93468	A peak
Total Area:				868906	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range