


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2018, Rack A, Plate 1, Well B10, 484354 FA
 [DD63C5F40728A6E8] Dec 15, 2025 10:14:53 Pressure = 74 bar (74 to 77)

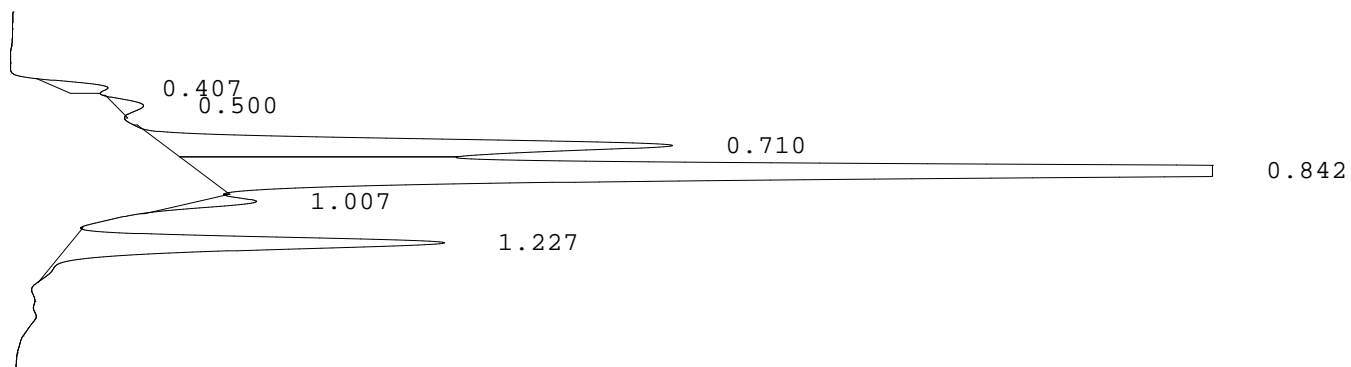

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	1.3%	15046	
2	0.500	F 0.59	0.9%	10636	
3	0.710	F 0.84	20.1%	228945	
4	0.842	F 0.99	62.7%	712635	Consistent with F
5	1.007	F 1.18	1.6%	18746	
6	1.227	A 1.01	13.3%	151314	A peak
Total Area:				1137322	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range