


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2029, Rack A, Plate 1, Well F09, 171704  
[8977D2B8BA2AAC6A] Dec 29, 2025 13:13:40 Pressure = 74 bar (74 to 76)

FA

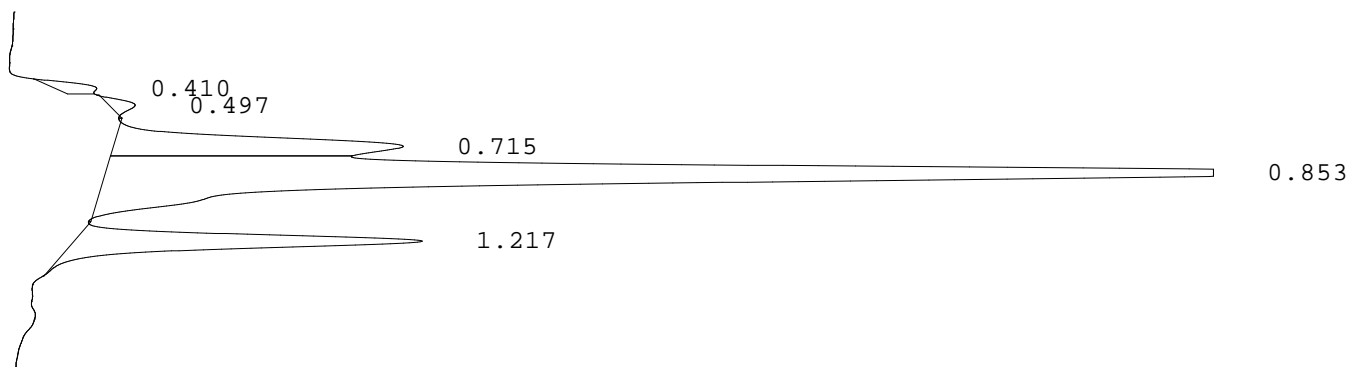

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.410	F 0.48	1.3%	13219	
2	0.497	F 0.58	0.9%	9936	
3	0.715	F 0.83	14.7%	154095	Acetylated F peak
4	0.853	F 0.99	68.9%	722090	Consistent with F
5	1.217	A 1.01	14.2%	149124	A peak

Total Area: 1048464

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range