


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2018, Rack A, Plate 1, Well E09, 486549
[9C7385A15077F197] Dec 15, 2025 11:27:38 Pressure = 74 bar (73 to 75)

FA

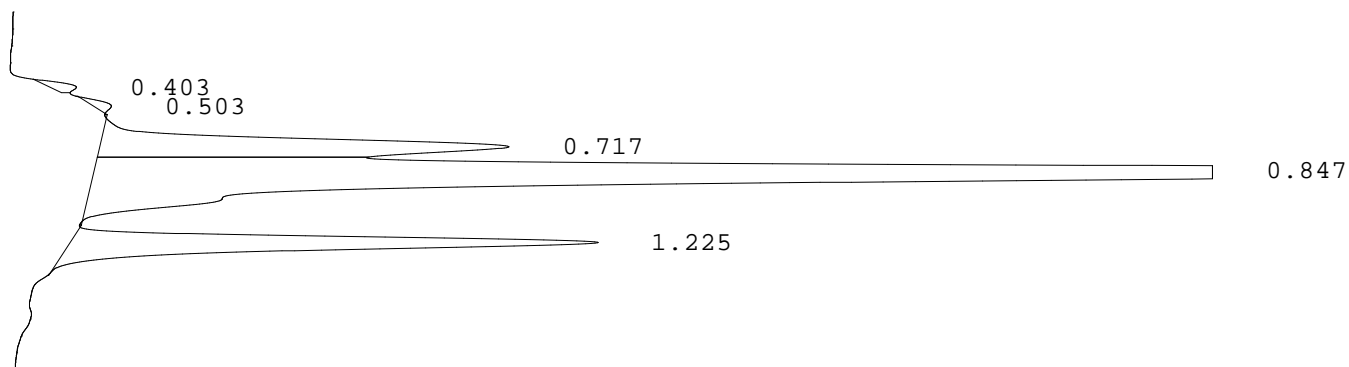

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.47	0.5%	7184	
2	0.503	F 0.59	0.5%	6306	
3	0.717	F 0.84	14.8%	204127	Acetylated F peak
4	0.847	F 0.99	68.6%	948350	Consistent with F
5	1.225	A 1.00	15.7%	216656	A peak

Total Area: 1382623

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range