


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2018, Rack A, Plate 1, Well B09, 486531
[996290A1527D7115] Dec 15, 2025 10:12:51 Pressure = 75 bar (74 to 77)

FA

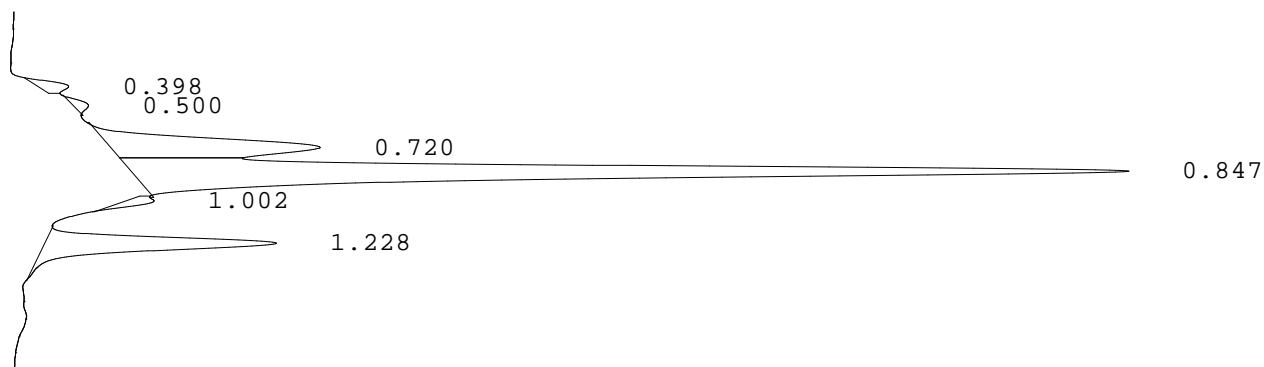

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.398	F 0.47	1.4%	9161	
2	0.500	F 0.59	0.8%	5347	
3	0.720	F 0.85	17.3%	109358	Acetylated F peak
4	0.847	F 1.00	64.0%	404835	Consistent with F
5	1.002	F 1.18	1.5%	9333	
6	1.228	A 1.02	15.0%	94628	A peak

Total Area: 632662

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range