


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1941, Rack A, Plate 1, Well A05, 170244-P
[DC311DCFB71CF935] Oct 09, 2025 11:24:55 Pressure = 67 bar (67 to 68)

FA

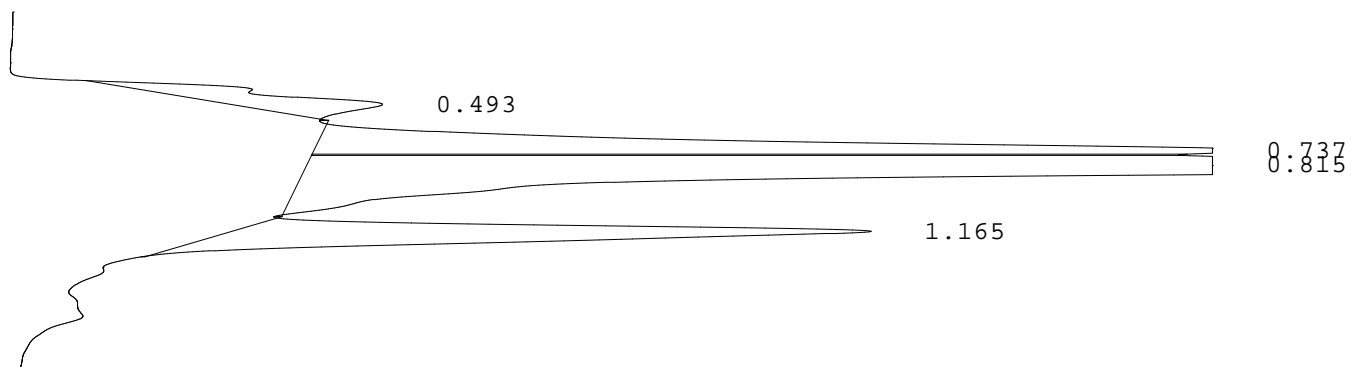

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.493	F 0.60	5.1%	104020	
2	0.737	F 0.89	19.7%	406049	
3	0.815	F 0.98	60.4%	1243908	Consistent with F
4	1.165	A 0.99	14.8%	305325	A peak
Total Area:				2059302	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range