


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2061, Rack A, Plate 1, Well A12, 489305
[CD73CF45FEED5B3F] Jan 30, 2026 10:23:48 Pressure = 91 bar (90 to 93)

FA

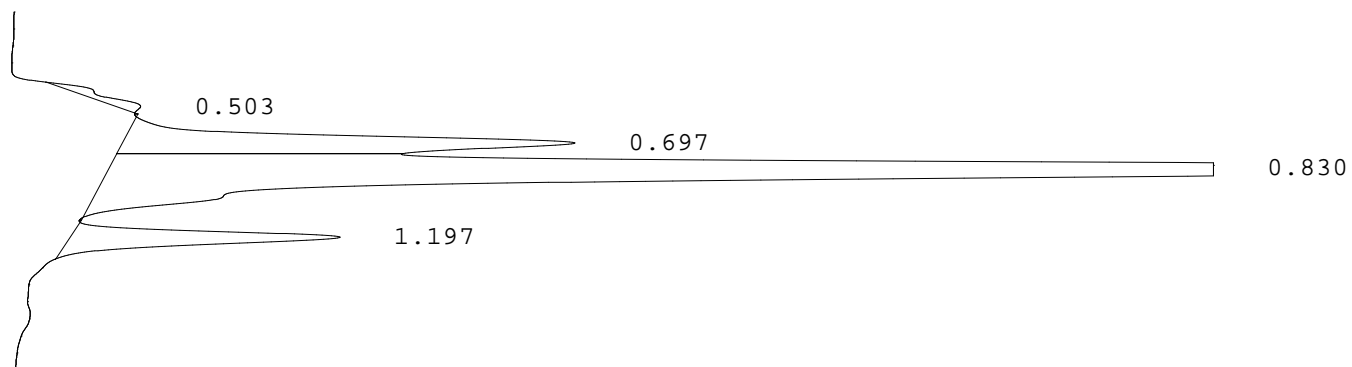

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.503	F 0.60	1.3%	17630	
2	0.697	F 0.83	16.5%	217013	Acetylated F peak
3	0.830	F 0.99	73.8%	968304	Consistent with F
4	1.197	A 1.01	8.3%	109276	A peak
Total Area:				1312223	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range