


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2051, Rack A, Plate 1, Well A03, 490379-P
[C9768D1AE9BFF9B7] Jan 20, 2026 14:51:58 Pressure = 79 bar (79 to 81)

FA

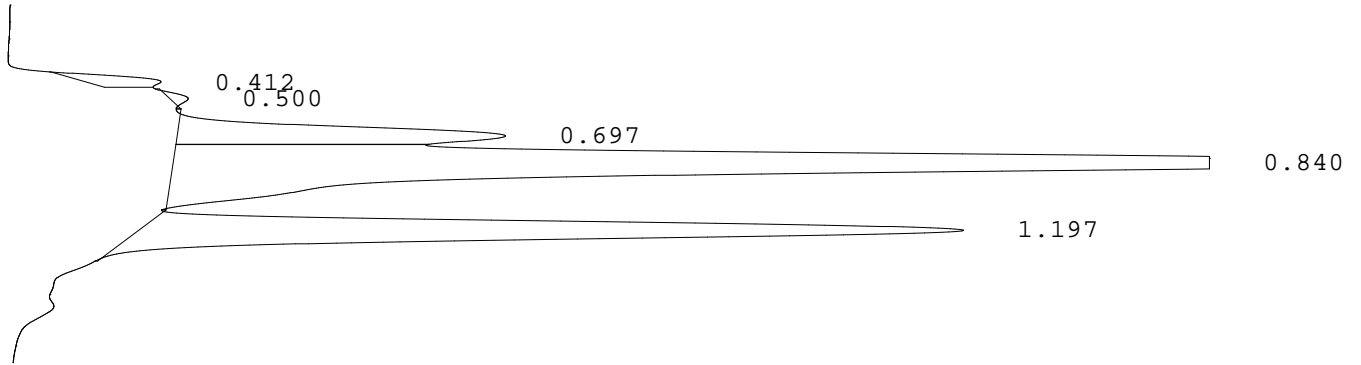

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.412	F 0.48	1.6%	24392	
2	0.500	F 0.59	0.5%	7035	
3	0.697	F 0.82	10.9%	166077	Acetylated F peak
4	0.840	F 0.99	58.1%	880664	Consistent with F
5	1.197	A 1.00	28.9%	438850	A peak - REVIEW

Total Area: 1517018

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range