


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2008, Rack A, Plate 1, Well F12, 171426
 [8863BB7173CFD995] Dec 09, 2025 13:21:15 Pressure = 72 bar (71 to 73)

FA

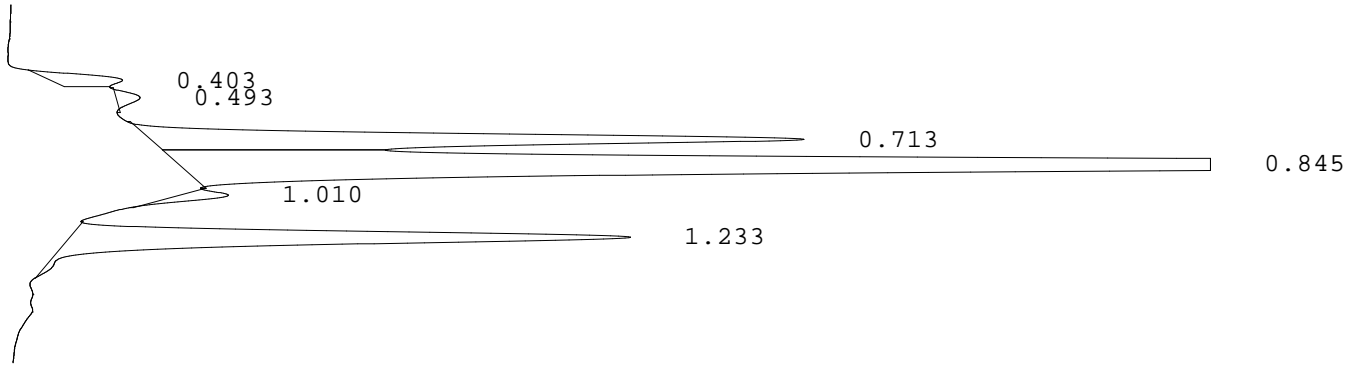

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.47	1.8%	23702	
2	0.493	F 0.57	0.7%	9314	
3	0.713	F 0.82	18.4%	237724	
4	0.845	F 0.98	60.5%	781495	Consistent with F
5	1.010	F 1.17	1.2%	15625	
6	1.233	A 1.01	17.3%	223223	A peak
Total Area:				1291083	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range