


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 1953, Rack A, Plate 1, Well B05, 859881  
[CD215E9F97C10CC2] Oct 21, 2025 10:47:38 Pressure = 66 bar (66 to 68)

FA

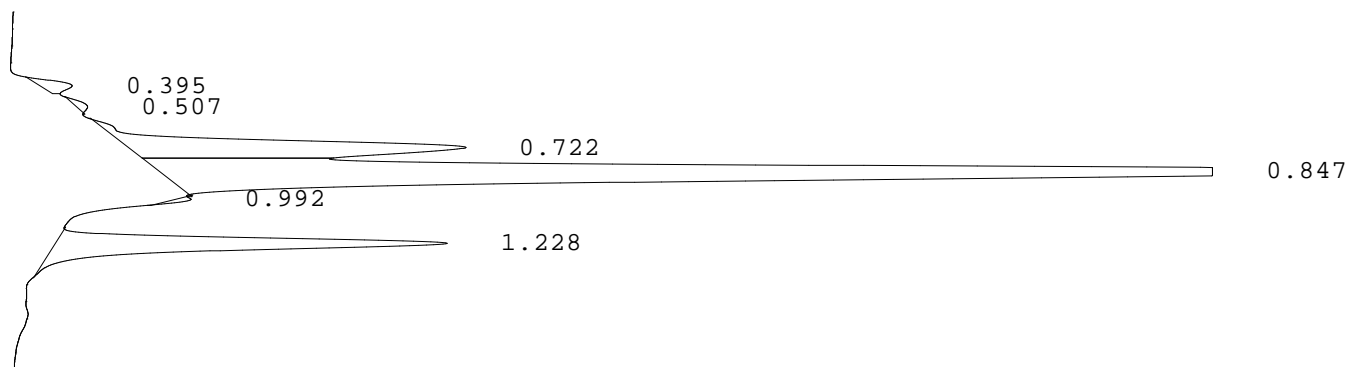

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.395	F 0.46	1.1%	9833	
2	0.507	F 0.59	0.4%	3960	
3	0.722	F 0.85	17.1%	156554	Acetylated F peak
4	0.847	F 0.99	64.8%	591900	Consistent with F
5	0.992	F 1.16	0.4%	3858	
6	1.228	A 1.00	16.1%	147483	A peak
Total Area:				913588	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range