


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2176, Rack A, Plate 1, Well D01, 493884
 [C83DAC417ECDB195] Jun 12, 2026 13:03:39 Pressure = 68 bar (68 to 70)

FA

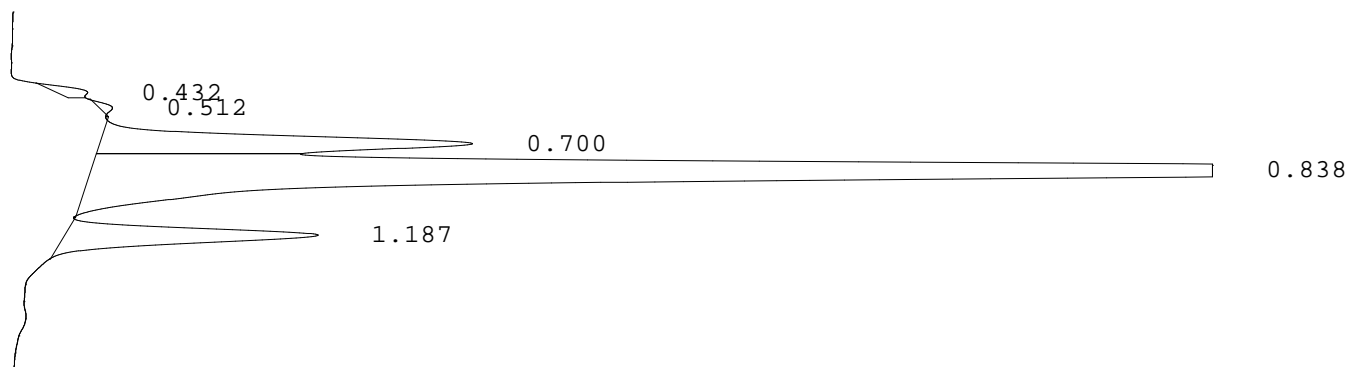

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.432	F 0.51	0.8%	9762	
2	0.512	F 0.61	0.4%	4361	
3	0.700	F 0.83	14.1%	172504	Acetylated F peak
4	0.838	F 0.99	75.3%	919394	Consistent with F
5	1.187	A 1.00	9.4%	114218	A peak
Total Area:				1220239	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range