


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2018, Rack A, Plate 1, Well G08, 171514
 [DD7380B17A57799D] Dec 15, 2025 12:16:09 Pressure = 72 bar (72 to 74)

FA

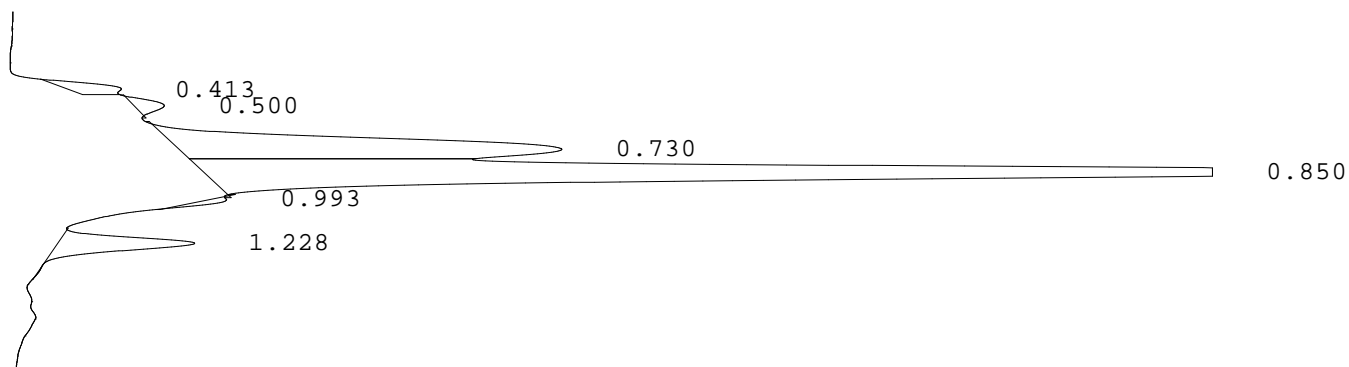

| PEAK | RT | REL RT | % CONC | AREA | COMMENT |
|-------------|-------|--------|--------|--------|-------------------|
| 1 | 0.413 | F 0.48 | 2.0% | 17376 | |
| 2 | 0.500 | F 0.58 | 1.3% | 11859 | |
| 3 | 0.730 | F 0.85 | 25.4% | 225364 | |
| 4 | 0.850 | F 0.99 | 64.2% | 569430 | Consistent with F |
| 5 | 0.993 | F 1.16 | 0.8% | 7279 | |
| 6 | 1.228 | A 1.01 | 6.2% | 55282 | A peak |
| Total Area: | | | | 886590 | |

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range