


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2197, Rack A, Plate 1, Well A04, 487102
[C83CD79FBF5DB11D] Jul 15, 2026 12:22:57

Pressure = 83 bar (83 to 85)

FA

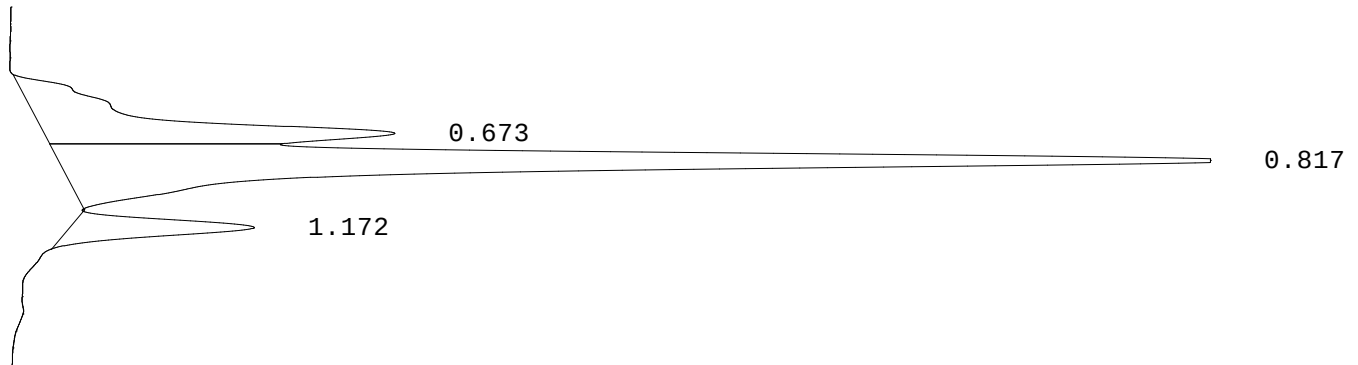

PEAK	RT	REL	RT	% CONC	AREA	COMMENT
1	0.673	F	0.81	24.5%	260750	
2	0.817	F	0.99	66.9%	712467	Consistent with F
3	1.172	A	1.01	8.6%	91347	A peak
Total Area: 1064564						

Codes: 1) Wide A peak
2) Area of A peak < 80%
3) Peak area greater than expected
4) Peak after A2
5) A1c > 10%
6) HbF or variant present
7) Total sample area too small/big
8) A2 is not within normal range