


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2025, Rack A, Plate 1, Well B04, 490111
[CD329038BB2A2EE2] Dec 23, 2025 11:33:18 Pressure = 77 bar (77 to 79)

FA

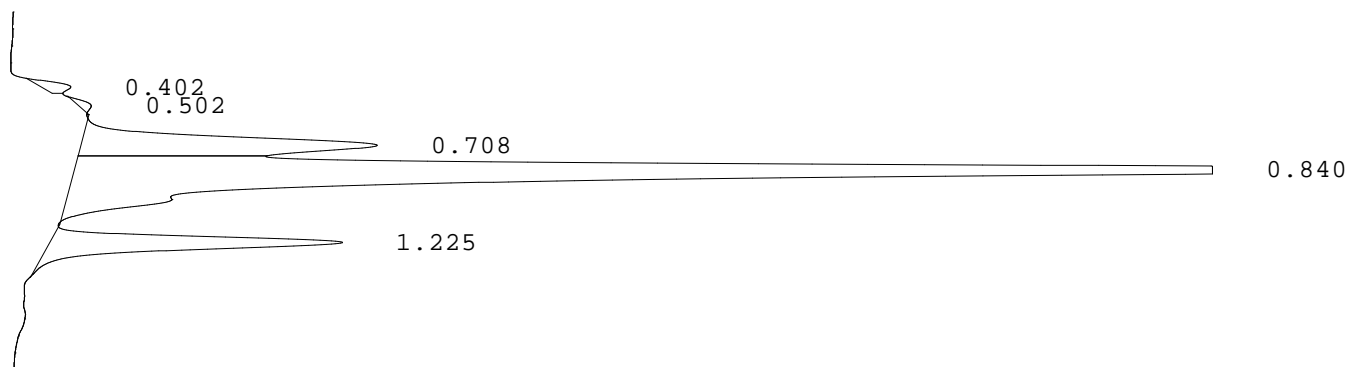

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.402	F 0.47	0.9%	8592	
2	0.502	F 0.59	0.4%	4401	
3	0.708	F 0.83	15.2%	151297	Acetylated F peak
4	0.840	F 0.99	71.6%	714252	Consistent with F
5	1.225	A 1.01	11.9%	118514	A peak
Total Area:				997056	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range