


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2156, Rack A, Plate 1, Well H11, 501509
[892CE287A0259115] May 26, 2026 14:42:43 Pressure = 65 bar (64 to 67)

FA

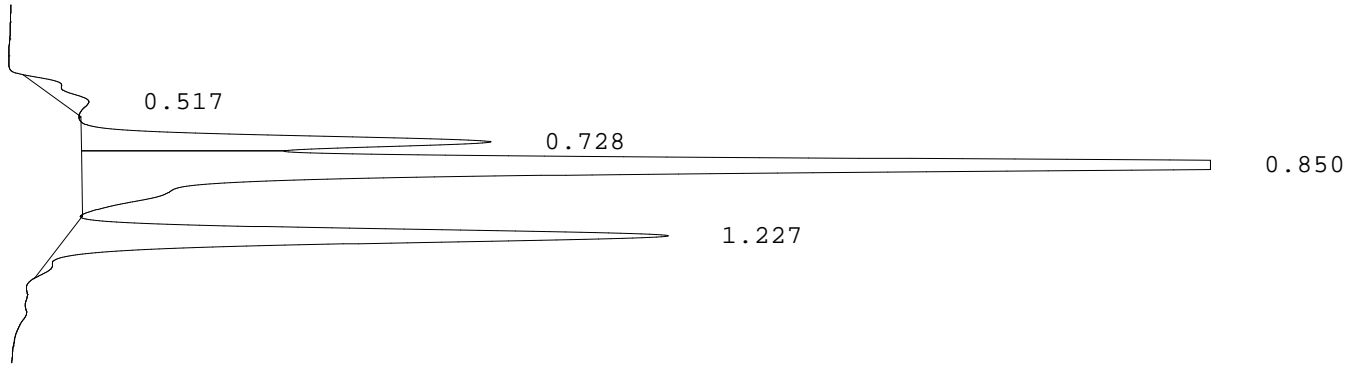

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.517	F 0.60	1.9%	22882	
2	0.728	F 0.84	13.5%	159531	Acetylated F peak
3	0.850	F 0.98	61.4%	722947	Consistent with F
4	1.227	A 1.01	23.1%	272512	A peak - REVIEW
Total Area:				1177872	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range