


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2027, Rack A, Plate 1, Well A02, 171597-P
 [9972C12DE4D57335] Dec 23, 2025 15:28:23 Pressure = 74 bar (74 to 76)

FA

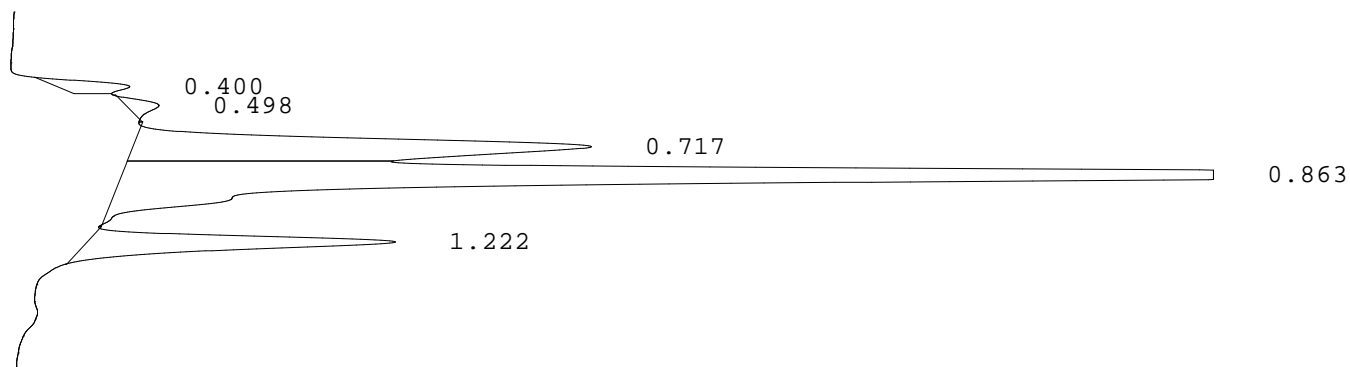

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.400	F 0.47	2.0%	22882	
2	0.498	F 0.59	1.2%	13590	
3	0.717	F 0.84	22.7%	261840	
4	0.863	F 1.01	63.1%	727848	Consistent with F
5	1.222	A 1.01	11.1%	127500	A peak
Total Area:				1153660	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range