


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2018, Rack A, Plate 1, Well D05, 486533
 [9877D1F407A02662] Dec 15, 2025 10:55:18 Pressure = 74 bar (73 to 75)

FA

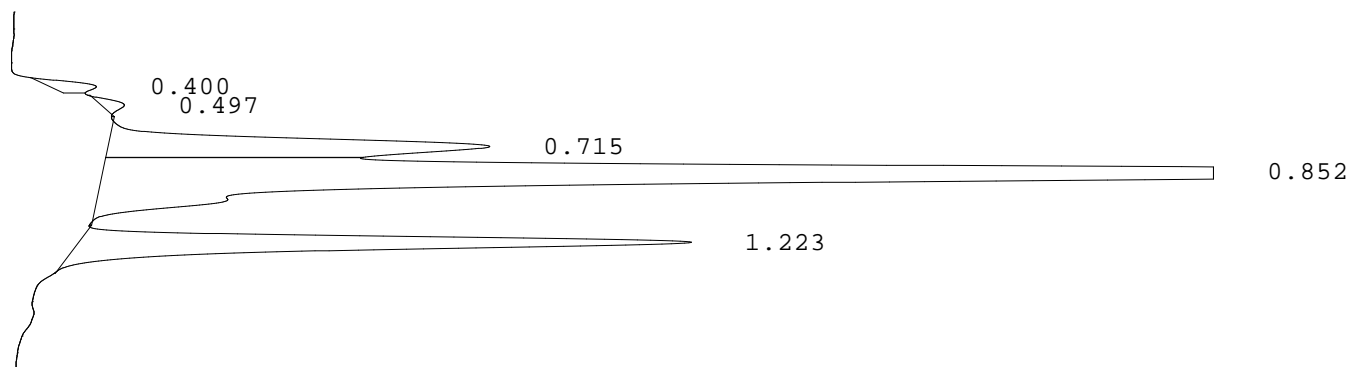

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.400	F 0.47	1.0%	13859	
2	0.497	F 0.58	0.6%	8339	
3	0.715	F 0.83	14.6%	195510	Acetylated F peak
4	0.852	F 0.99	65.1%	873361	Consistent with F
5	1.223	A 1.00	18.7%	250601	A peak
Total Area:				1341670	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range