


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2018, Rack A, Plate 1, Well D08, 486538  
 [CD6395A1505FF917] Dec 15, 2025 11:01:22 Pressure = 73 bar (72 to 75)

FA

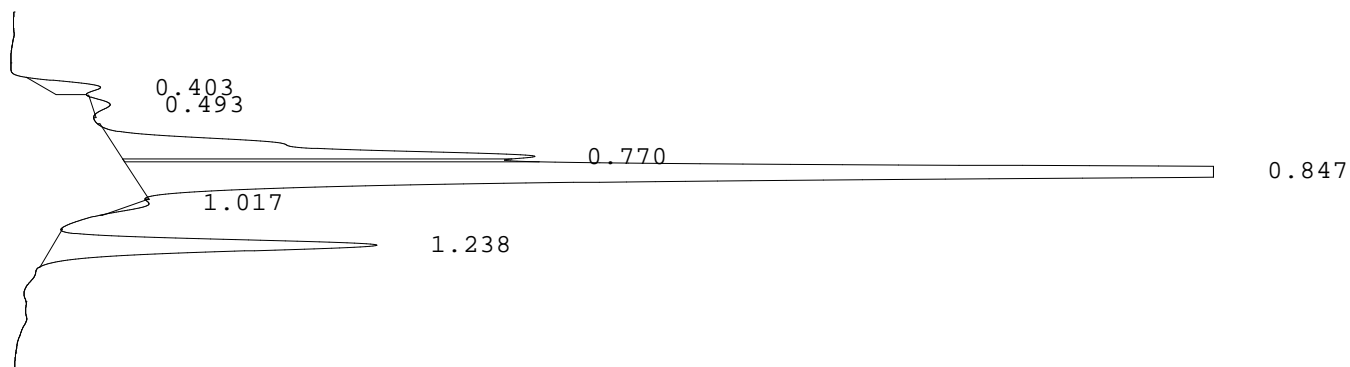

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.47	1.7%	18706	
2	0.493	F 0.58	0.6%	6271	
3	0.770	F 0.90	17.4%	188746	Acetylated F peak
4	0.847	F 0.99	68.4%	743202	Consistent with F
5	1.017	F 1.19	0.5%	5450	
6	1.238	A 1.01	11.5%	124441	A peak
Total Area:				1086816	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range