


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1993, Rack A, Plate 1, Well F02, 482088
 [8C22B9D2F7920EE0] Nov 25, 2025 12:40:31 Pressure = 68 bar (67 to 69)

FA

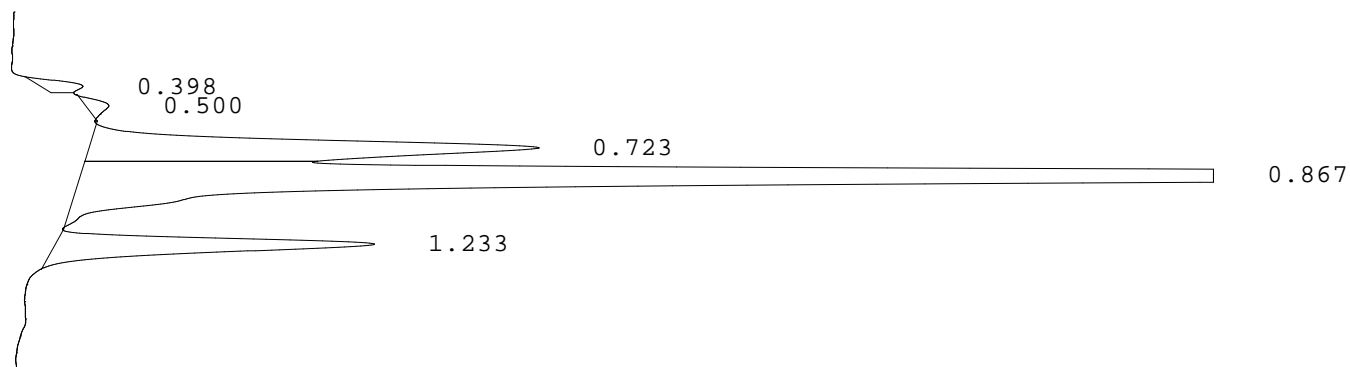

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.398	F 0.46	0.9%	13209	
2	0.500	F 0.58	0.7%	9968	
3	0.723	F 0.84	17.0%	238473	Acetylated F peak
4	0.867	F 1.01	71.6%	1003759	Consistent with F
5	1.233	A 1.00	9.7%	135632	A peak
Total Area:				1401041	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range