


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2156, Rack A, Plate 1, Well F02, 501680
[DC79A2D2F770CCCA] May 26, 2026 13:34:00 Pressure = 66 bar (65 to 67)

FA

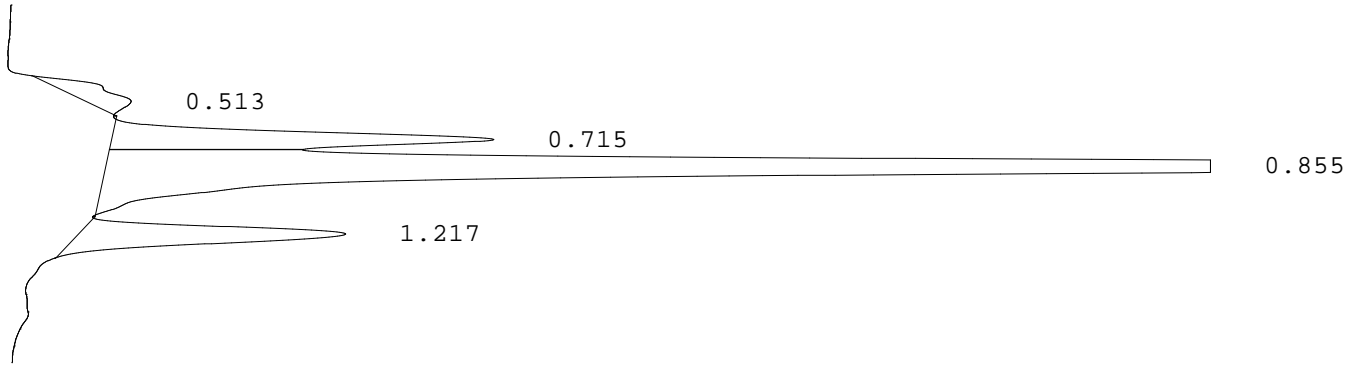

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.513	F 0.59	3.1%	38358	
2	0.715	F 0.82	13.7%	171282	Acetylated F peak
3	0.855	F 0.98	72.3%	904944	Consistent with F
4	1.217	A 1.01	10.9%	136508	A peak
Total Area:				1251092	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range