


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2137, Rack A, Plate 1, Well B11, 498945
[CD220EEACFE371B5] Apr 30, 2026 12:16:47 Pressure = 63 bar (62 to 64)

FA

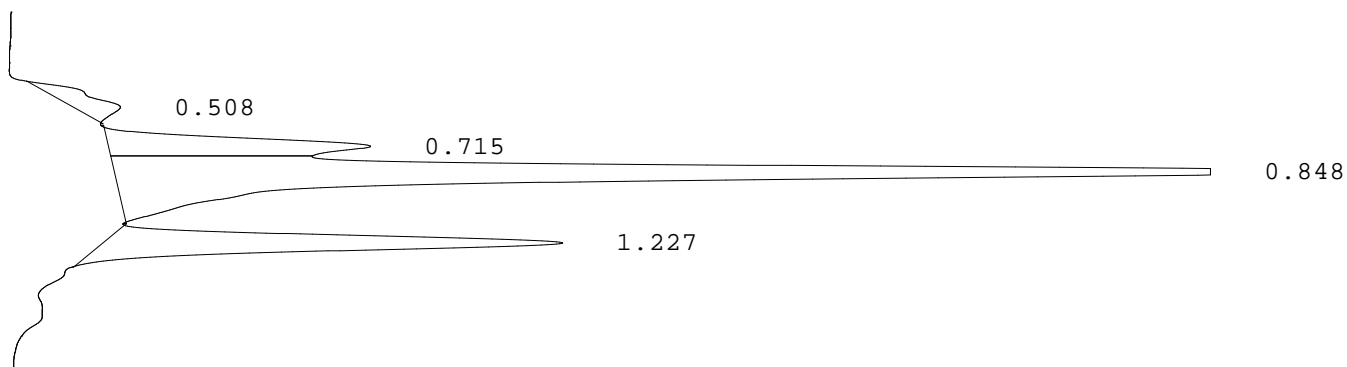

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.508	F 0.59	3.5%	36341	
2	0.715	F 0.83	12.5%	129229	Acetylated F peak
3	0.848	F 0.99	63.0%	651212	Consistent with F
4	1.227	A 1.01	21.0%	217639	A peak - REVIEW

Total Area: 1034421

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range