


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2073, Rack A, Plate 1, Well D05, 489337
 [D827245B3451711F] Feb 13, 2026 13:54:40 Pressure = 52 bar (52 to 53)

FA

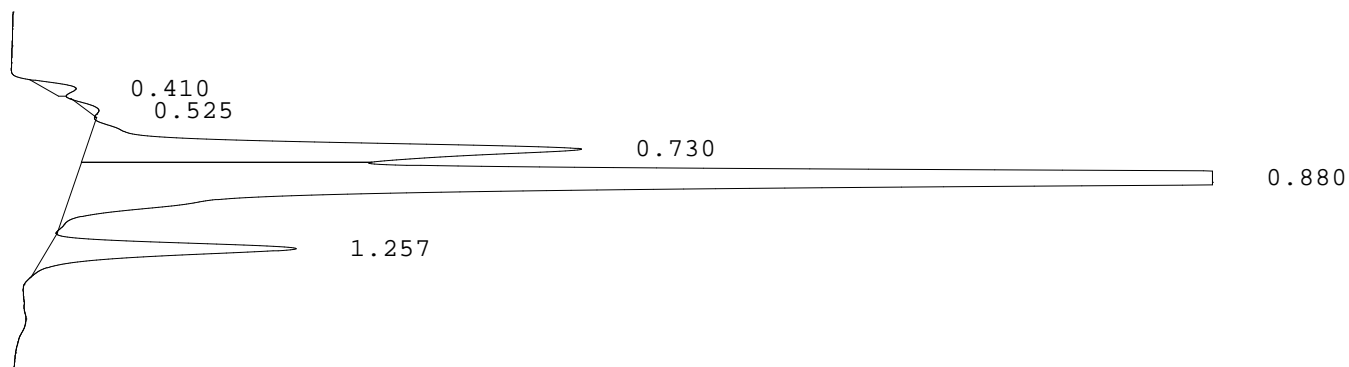

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.410	F 0.46	0.7%	9607	
2	0.525	F 0.59	0.3%	4732	
3	0.730	F 0.82	18.0%	253579	Acetylated F peak
4	0.880	F 0.99	74.0%	1045260	Consistent with F
5	1.257	A 1.00	7.0%	99161	A peak
Total Area:				1412339	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range