


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 1982, Rack A, Plate 1, Well D12, 482218  
 [CD76E652F487DB97] Nov 19, 2025 12:12:42 Pressure = 68 bar (68 to 70)

FA

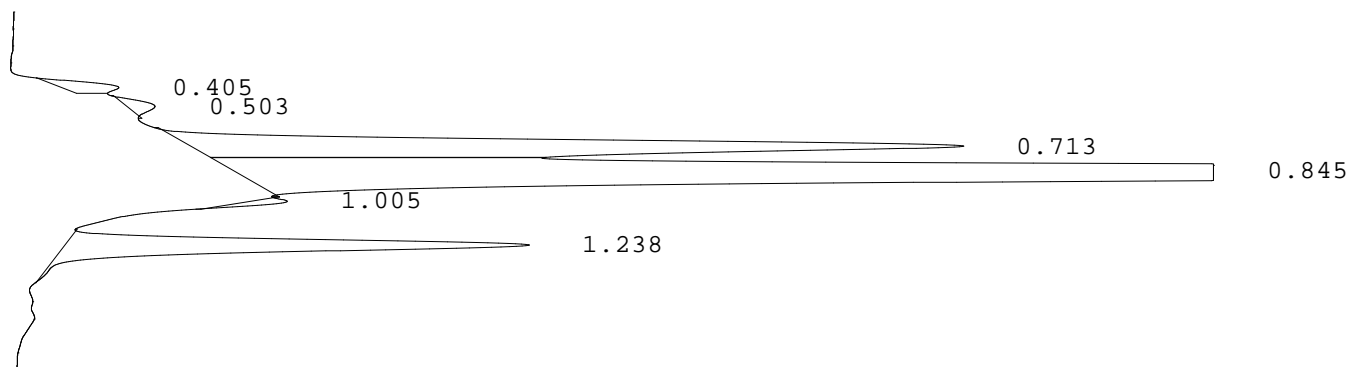

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.47	1.0%	17509	
2	0.503	F 0.58	0.6%	10967	
3	0.713	F 0.83	18.0%	325176	Acetylated F peak
4	0.845	F 0.98	70.1%	1263517	Consistent with F
5	1.005	F 1.17	0.6%	10143	
6	1.238	A 1.00	9.7%	175037	A peak
Total Area:				1802349	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range