


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1982, Rack A, Plate 1, Well F01, 482076
 [CD36A7494B5806EA] Nov 19, 2025 12:41:00 Pressure = 68 bar (67 to 70)

FA

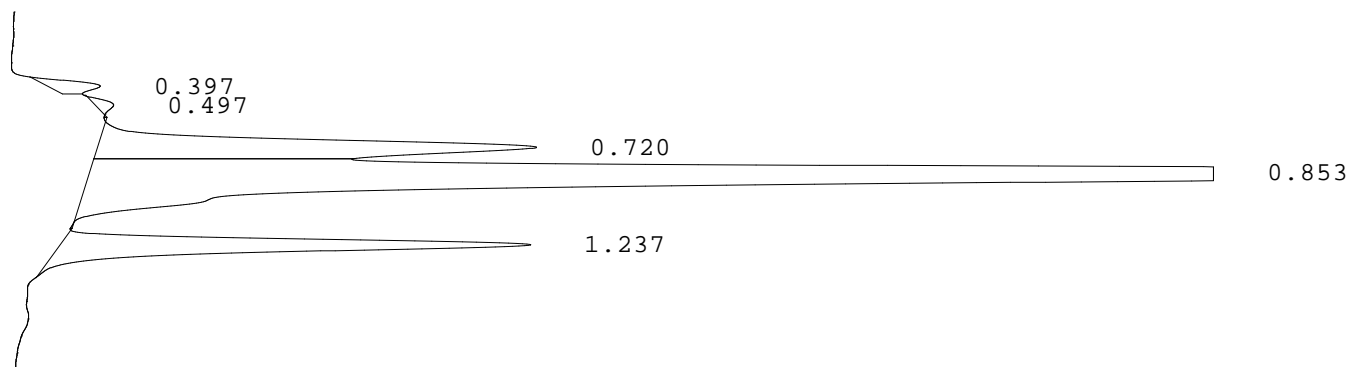

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.397	F 0.46	1.1%	16621	
2	0.497	F 0.58	0.5%	6913	
3	0.720	F 0.83	14.9%	216804	Acetylated F peak
4	0.853	F 0.99	70.9%	1030791	Consistent with F
5	1.237	A 1.00	12.6%	183617	A peak
Total Area:				1454746	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range