


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1359, Rack A, Plate 1, Well H09, 27401
 [98D9E456DC78C8E2] Apr 03, 2024 12:45:02

Pressure = 59 bar (59 to 59)

FA

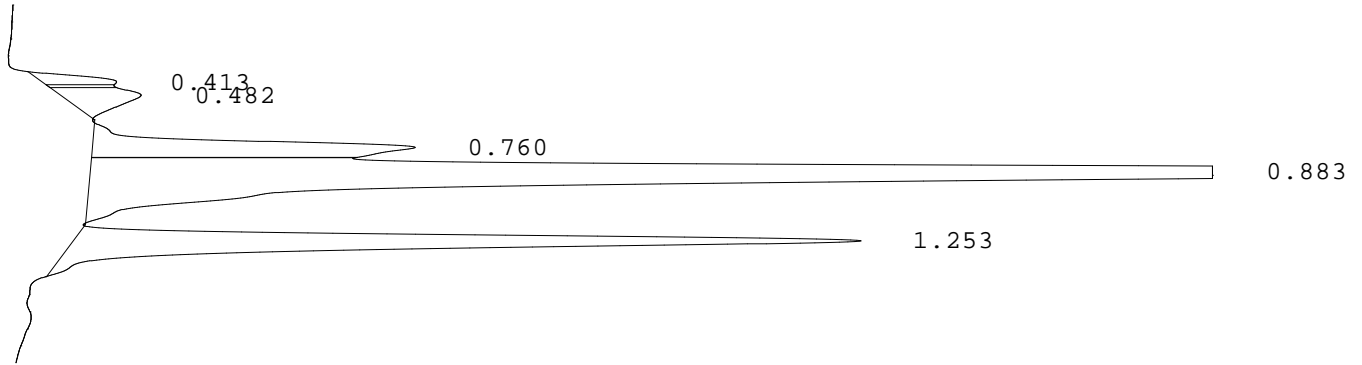

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.413	F 0.46	1.6%	24661	
2	0.482	F 0.54	3.2%	48790	
3	0.760	F 0.85	9.7%	148290	Acetylated F peak
4	0.883	F 0.99	64.3%	984514	Consistent with F
5	1.253	A 1.00	21.2%	324635	A peak - REVIEW
Total Area:				1530890	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range