


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2018, Rack A, Plate 1, Well C03, 484360
 [897794A152DF7B95] Dec 15, 2025 10:24:59 Pressure = 74 bar (74 to 77)

FA

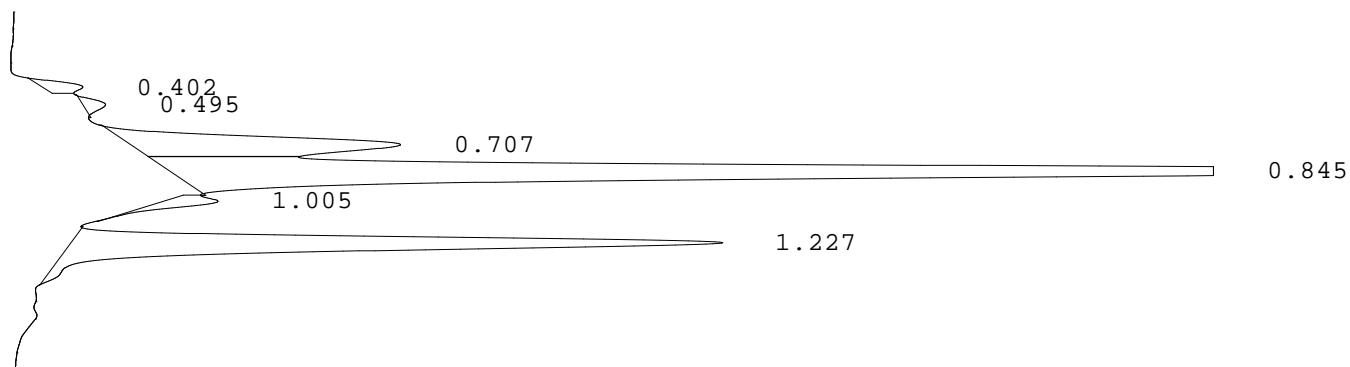

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.402	F 0.47	1.2%	12296	
2	0.495	F 0.58	0.8%	8245	
3	0.707	F 0.83	13.4%	140103	Acetylated F peak
4	0.845	F 0.99	56.5%	590182	Consistent with F
5	1.005	F 1.18	1.9%	20211	
6	1.227	A 1.01	26.2%	273039	A peak - REVIEW
Total Area:				1044076	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range