


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1880, Rack A, Plate 1, Well A01, 457233
[CD3072FC1884F3B5] Aug 05, 2025 09:57:51 Pressure = 64 bar (63 to 66)

FA

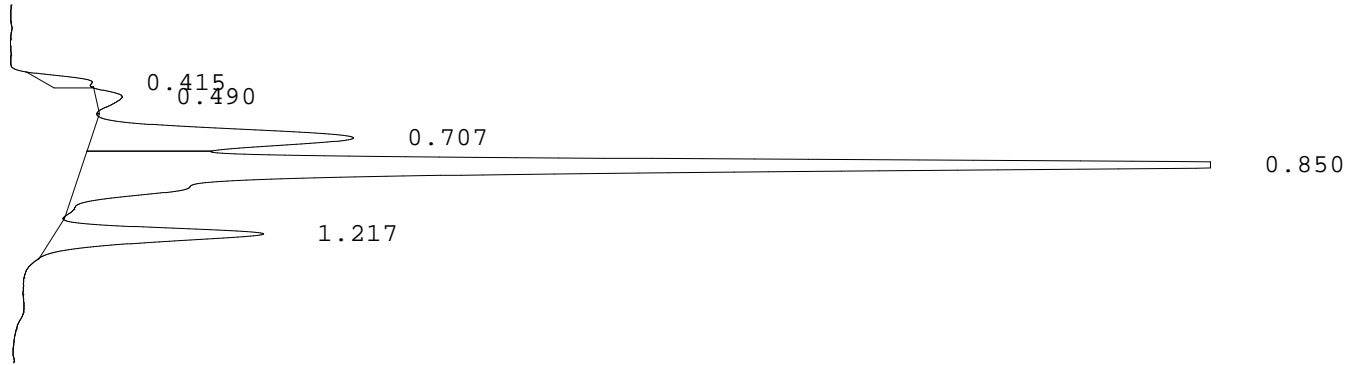

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.415	F 0.49	1.9%	15754	
2	0.490	F 0.58	1.4%	11512	
3	0.707	F 0.84	17.3%	146715	Acetylated F peak
4	0.850	F 1.01	68.9%	584877	Consistent with F
5	1.217	A 1.01	10.6%	89538	A peak
Total Area:				848396	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range