


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2068, Rack A, Plate 1, Well D09, 492219
[C922717B3306AEC0] Feb 10, 2026 11:54:35 Pressure = 96 bar (95 to 99)

FA

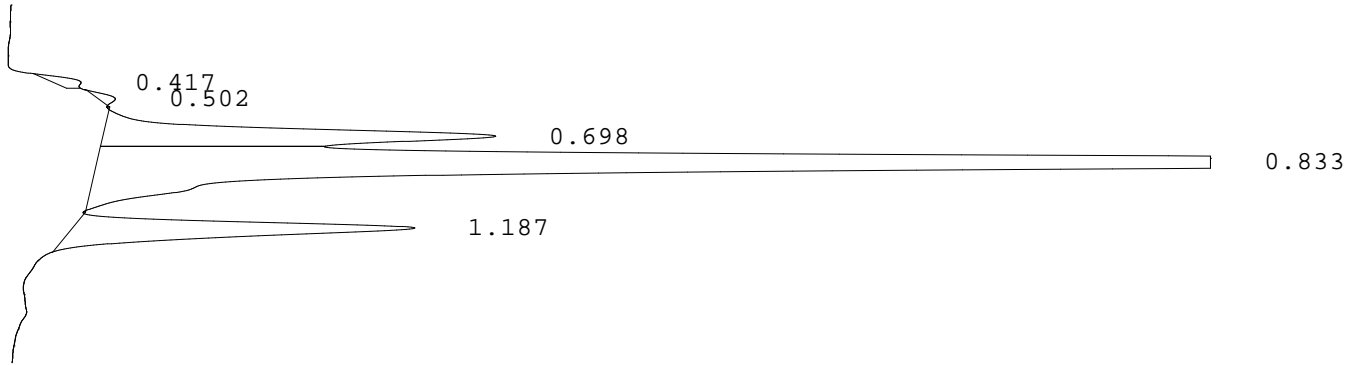

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.417	F 0.49	0.7%	8546	
2	0.502	F 0.59	0.4%	5421	
3	0.698	F 0.83	14.2%	181204	Acetylated F peak
4	0.833	F 0.99	72.9%	933062	Consistent with F
5	1.187	A 1.01	11.8%	151130	A peak
Total Area:				1279363	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range