


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2153, Rack A, Plate 1, Well C01, 501656
[DC3DB45E43AD9B15] May 21, 2026 11:06:27 Pressure = 68 bar (67 to 70)

FA

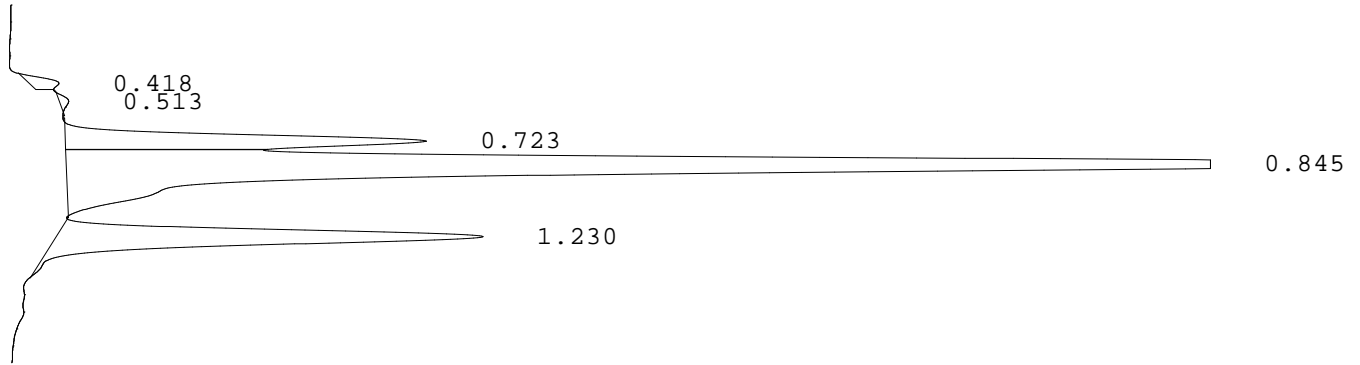

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.418	F 0.49	0.9%	9418	
2	0.513	F 0.60	0.3%	3789	
3	0.723	F 0.85	12.9%	139717	Acetylated F peak
4	0.845	F 0.99	67.7%	733820	Consistent with F
5	1.230	A 1.02	18.2%	197463	A peak
Total Area:				1084207	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range