


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2018, Rack A, Plate 1, Well H02, 171520  
 [9C63C5E42F28044A] Dec 15, 2025 12:28:16 Pressure = 72 bar (72 to 74)

FA

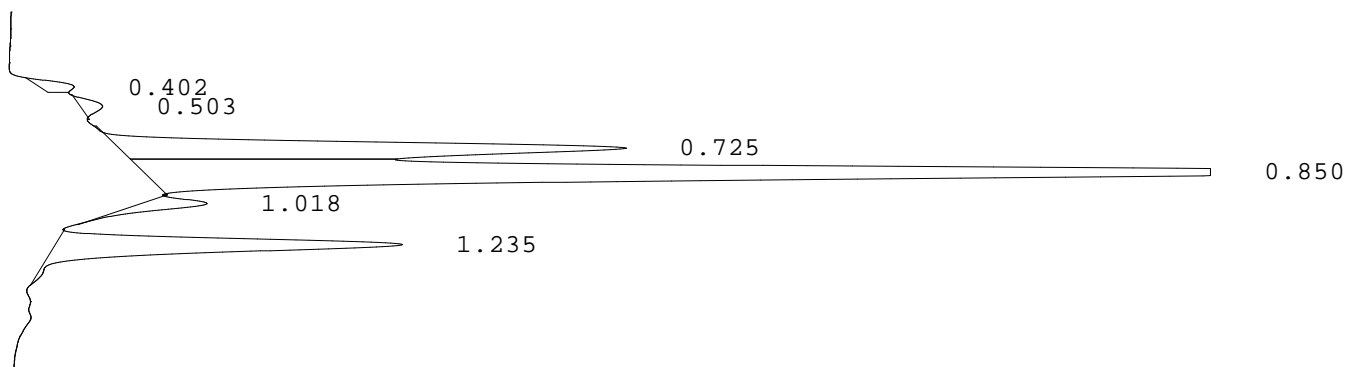

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.402	F 0.47	1.1%	10454	
2	0.503	F 0.59	1.0%	9154	
3	0.725	F 0.85	22.3%	213507	
4	0.850	F 0.99	58.1%	556703	Consistent with F
5	1.018	F 1.19	2.5%	24202	
6	1.235	A 1.01	15.0%	143435	A peak
Total Area:				957455	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range