


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2003, Rack A, Plate 1, Well F02, 484318
 [8D33EFA4254F5917] Dec 03, 2025 12:14:58 Pressure = 72 bar (72 to 74)

FA

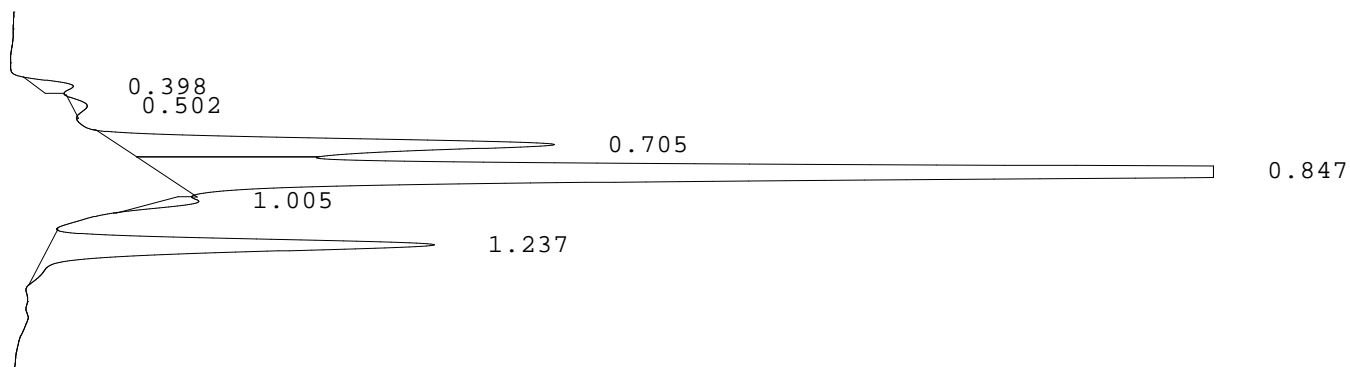

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.398	F 0.46	1.1%	11879	
2	0.502	F 0.58	0.5%	5919	
3	0.705	F 0.82	16.8%	185036	Acetylated F peak
4	0.847	F 0.99	66.2%	730766	Consistent with F
5	1.005	F 1.17	1.2%	13198	
6	1.237	A 1.00	14.2%	157034	A peak
Total Area:				1103832	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range